MODE OF ACTION

MECHANICAL DEBRIDEMENT ALONE OR WITH PERISOLV®

BEFORE

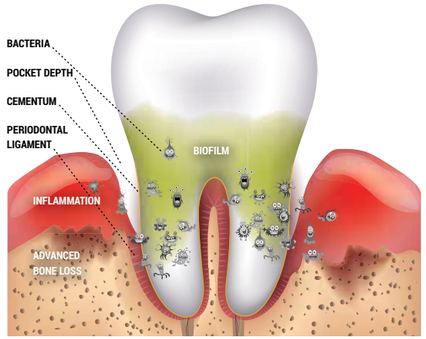

AFTER

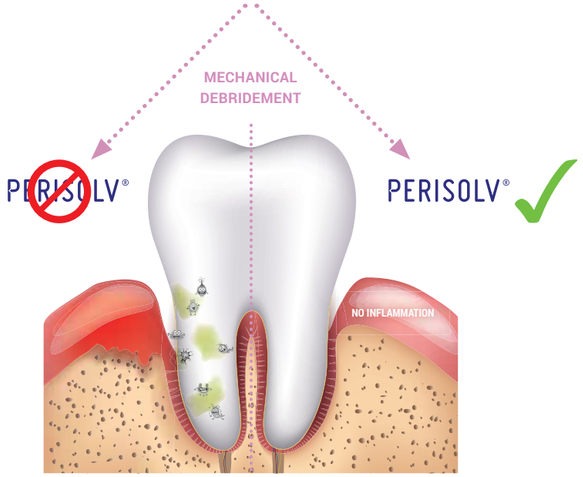

SIMPLE APPLICATION



1. CONNECT



2. MIX



3. CANNULA

4. APPLY

30 sec

5. WAIT

Repeat 3-5

6. START

MORE CLINICAL CASES AVAILABLE AT
www.regedent.com

LITERATURE

1. Data on file.
2. Guarnelli ME et al. 'Professional local administration of chloramine-based treatment in conjunction with ultrasonic mechanical instrumentation: clinical outcomes in patients with deep periodontal pockets persisting following active non-surgical therapy'. Minerva Stomatologia, April 2015; Vol. 64 suppl. 1 al No. 2: 158-159.
3. Data on file.

PERISOLV® is a registered trademark and is manufactured by RLS Global AB, Neongatan 5, SE-431 53 Mölndal.

SHOW BIOFILM THE „RED" CARD

ELIMINATION OF THE BIOFILM IS KEY FOR THE TREATMENT SUCCESS OF PERIODONTITIS, PERI-IMPLANT MUCOSITIS, AND PERI-IMPLANTITIS.

Art. 8131.902EN, 2018-01-01

REGEDENT AG
Zollikerstrasse 144 | CH-8008 Zürich
Tel. +41 (0) 44 700 37 77
info@regendent.com | www.regedent.com

A NEW APPLICATION

FOR PERIODONTAL AND PERI-IMPLANT INFLAMMATION

Periodontitis, peri-implant mucositis and peri-implantitis are bacterial inflammations with similar symptoms. The underlying cause of all three indications, which progress in a similar way, is bacterial plaque forming a biofilm, rich in pathogenic bacteria. The softening of the biofilm and effective elimination of the bacteria is the key prerequisite for successful treatment of these conditions.

PERISOLV® is a new cleaning gel used in addition to mechanical debridement.

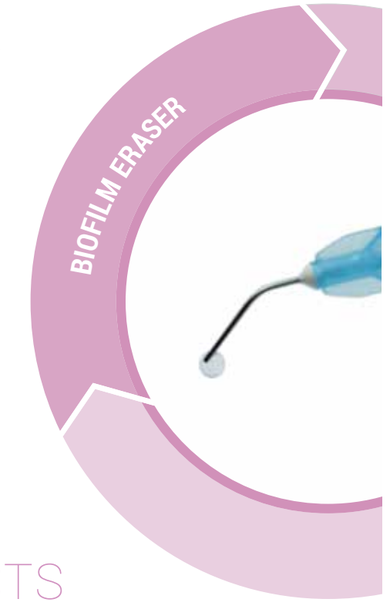

PERISOLV®-EFFECTS

- ELIMINATION OF THE BIOFILM*
- IMPROVED MUCOSITIS TREATMENT[1]
- REDUCTION OF POCKET DEPTH EVEN IN PERSISTENT POCKETS[2, 3]

* Enhancing bacterial removal by mechanical debridement.

TREATMENT OF PERI-IMPLANTMUCOSITIS

CASE BY PROF. VINCENZO IORIO-SICILIANO, UNIVERSITY OF CATANZARO, ITALY

Implant with probing depth (PD) ≤ 5mm and BOP+.

Application of PERISOLV® before non-surgical treatment.

Biofilm removal using a sonic scaler with PEEK tip.

6 MONTHS AFTER TREATEMENT

Probing depth (PD) after 6 months observation time.

TREATMENT OF A FURCATION DEFECT

CASE BY PROF. VINCENZO-IORIO-SICILIANO, UNIVERSITY OF CATANZARO, ITALY

1. A PD of 5 mm was noted.
2. A class-II furcation defect was recorded.

3. First application of PERISOLV®.
4. Scaling was performed using an ultrasonic device.

5. Second application of PERISOLV®.
6. Root planing was performed.

6 MONTHS AFTER TREATEMENT

7. A PD of 3 mm was reported.
8. A class-I furcation defect with BOP- was recorded.